



GlyCLICK®

Biotin 2 mg

STORE AT

DIFFERENT
TEMPERATURES



FOR RESEARCH USE ONLY

Instructions for Use

GlyCLICK® Biotin 2 mg (L1-A01-200)
Process 2 mg IgG

DOWNLOAD INSTRUCTIONS FOR USE



www.genovis.com/ifu-L1-A01-200

Site-specific Conjugation of IgG with Biotin

GlyCLICK is a site-specific conjugation technology for IgG using Fc N-glycan remodeling and click chemistry. The technology generates stable and homogenous antibody conjugates from several species and subclasses. Fc N-glycan remodeling by deglycosylation of the antibody allows for site-specific conjugation using robust click chemistry, resulting in a degree of labeling (DOL) or drug-antibody ratio (DAR) of 2.

GlyCLICK Biotin is available for site-specific labeling of 250 µg or 2 mg IgG with biotin. The conjugation is performed by combining enzymatic steps and copper-free click chemistry to covalently link the label to the Fc domain of the IgG. All steps are performed under physiological conditions, thus maintaining the quality of the antibody. The site-specific conjugation on the Fc domain preserves the affinity of the antigen-binding sites.

GlyCLICK Biotin 2 mg contains all reagents needed to conjugate 2 mg IgG. The conjugation is performed in four steps:

1. **Deglycosylation:** GlycINATOR Immobilized hydrolyzes the N-glycans on the Fc-part of the IgG to the inner GlcNAc.
2. **Azide Activation:** Azide attachment on the GlcNAc using GalT (Y289L)* and UDP-GalNAz*.
3. **Click Reaction:** The azide-activated antibody reacts with a DIBO-alkyne label in a strain-promoted, copper-free click reaction (SPAAC) to form a stable and homogenous antibody conjugate.
4. **Purification:** Excess DIBO-alkyne label is removed by using a desalting column.

YOU MIGHT ALSO BE INTERESTED IN

GlycINATOR™ Immobilized

Immobilized enzyme for deglycosylation of IgG in spin columns

GlyCLICK® Azide Activation

Site-specific conjugation of IgG with azide-alkyne click chemistry


GlyCLICK® Fluorophore

Site-specific conjugation of IgG with Alexa Fluor® 488, 555 or 647

GlyCLICK® DFO


Site-specific conjugation of IgG with DFO

* GalT (Y289L) and UDP-GalNAz are components of SiteClick™ and are provided under an intellectual property license from Life Technologies Corporation. The trademark SiteClick™ is the property of Life Technologies Corporation.

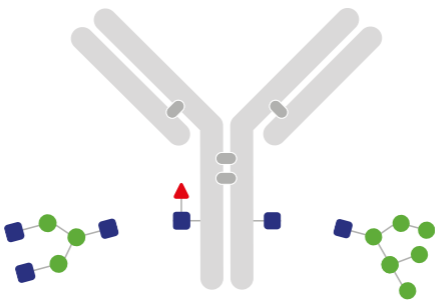


1. Deglycosylation

GlycINATOR Immobilized

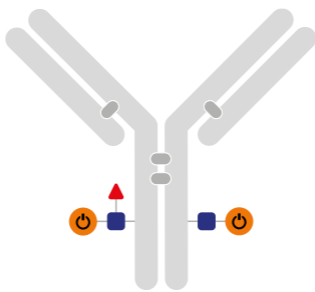

2. Azide Activation

GalT + UDP-GalNAz

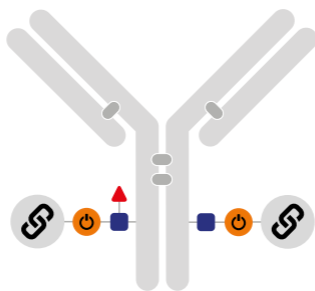

3. Click Reaction

DIBO-modified label: Biotin

4. Purification

Figure 1. Schematic overview of the GlyCLICK technology for biotin conjugation.

Preparations

Important Information

Before you begin, briefly centrifuge tubes. Always wear suitable laboratory protective clothing and gloves when handling the reagents. **Keep in mind:** Sodium azide must be avoided throughout the protocol.

- Let the GlycINATOR Immobilized and the Desalting Spin columns equilibrate to room temperature before use.
- Use lids and bottom caps during the incubation.
- Before centrifugation, remove the bottom cap and loosen the lid (do *not* remove the lid).

Additional Materials Required

- IgG in 1×TBS, pH 7.4, free of carrier proteins and/or azide. 2 mg of IgG in a maximum volume of 250 µl. To adjust the antibody solution, please follow “Guidance for Concentration and Buffer Exchange”. 20×TBS, a desalting spin column (0.5 ml, 40K) for buffer exchange and an antibody concentrator (0.5 ml, 50K) are provided for convenience.
- 1×TBS: 10 ml 1×TBS is prepared by adding 0.5 ml of 20×TBS to 9.5 ml of ddH₂O. Vortex briefly to mix.
- Centrifuge tubes: 1.5-2 ml and 15 ml.
- Dimethyl sulfoxide (DMSO) for reconstitution of biotin.
- ddH₂O.

Guidance for Concentration and Buffer Exchange

It is advisable to start with more IgG than 2 mg if concentration and/or buffer exchange of the sample is needed prior to “1. Deglycosylation: Modification of the N-glycan on the Antibody Fc Domain”.

A. Concentration Step

This step **is required if:**

- The volume of the IgG is more than 250 µl.

If the sample volume is 250 µl but needs a buffer exchange (if it contains phosphate or azide), concentrate the sample to < 150 µl and then follow the steps in section “B. Buffer Exchange”.

- A.1 Add 500 µl of ddH₂O to the Antibody concentrator (0.5 ml, 50K) and cap the device as shown in Figure 2.

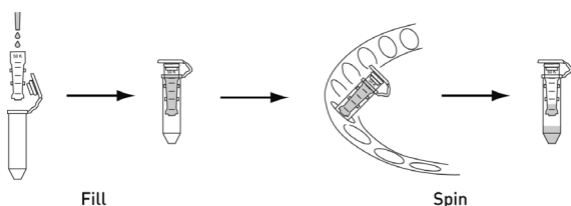


Figure 2. Antibody concentration step.

- A.2 Centrifuge at $5000\times g$ for 6 min. **Make sure that the cap strap and one membrane panel of the concentrator face the center of the rotor** (Fig. 2).
- A.3 Discard the flow-through.
- A.4 Add the IgG solution to the Antibody concentrator.
- A.5 Centrifuge at $5000\times g$ for 2-6 min. **Make sure that the cap strap and one membrane panel of the concentrator face the center of the rotor** (Fig. 2).

Note: *If the IgG volume in the concentrator is more than $150\mu\text{l}$ and the sample needs a buffer exchange, centrifuge for an additional 2 min at $5000\times g$, or until the appropriate volume is achieved.*


- A.6 Invert the Antibody concentrator into a new collection tube as shown in Figure 2.
- A.7 Centrifuge at $1000\times g$ for 3 min to collect the concentrated IgG. After collection, the volume of concentrated IgG should be approximately $100\text{-}150\mu\text{l}$ in the collection tube.

B. Buffer Exchange

This step **is required if:**

- The IgG is in another buffer than $1\times\text{TBS}$, and/or
- The IgG is in a buffer containing azide

- B.1 Let the Desalting Spin column (0.5 ml , 40K) equilibrate to room temperature before use. Break off the bottom closure of the Desalting Spin column. Loosen the lid (do not remove the lid).
- B.2 Place the column in a microcentrifuge tube and centrifuge at $700\times g$ for 1 min to remove the storage solution.
- B.3 Discard the flow-through and place the column in the microcentrifuge tube.
- B.4 Add $300\mu\text{l}$ of $1\times\text{TBS}$ on top of the resin. Centrifuge the column at $700\times g$ for 1 min and discard the flow-through.
- B.5 Perform step B.4 two additional times. The last time, centrifuge for 2 min.
- B.6 Blot the bottom of the column to remove excess liquid. Place the column in a new microcentrifuge tube.
- B.7 Apply the IgG solution ($100\text{-}150\mu\text{l}$) on top of the resin.
- B.8 Centrifuge at $700\times g$ for 2 min and collect the flow-through containing the antibody in $1\times\text{TBS}$.

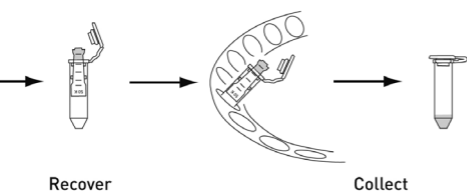

Site-specific Conjugation of IgG with Biotin

1. Deglycosylation: Modification of the N-glycan on the Antibody Fc Domain

Make sure that the antibody solution is 2 mg IgG in 250 μ l of 1 \times TBS (pH 7.4, without azide).

Time required: 15 min hands-on, 120 min hands-off.

Materials from kit:

- 1 \times TBS (prepared from 20 \times TBS)
 - Spin column with GlycINATOR Immobilized
- 1.1 Let the GlycINATOR Immobilized column equilibrate to room temperature before use. Break off the bottom cap of the GlycINATOR Immobilized column (save the cap) and place the column in a microcentrifuge tube. Loosen the lid.
 - 1.2 Centrifuge at 200 \times g for 1 min to remove the storage solution. Discard the flow-through.
 - 1.3 Place the column in the microcentrifuge tube.
 - 1.4 Add 300 μ l 1 \times TBS on top of the resin. Centrifuge the column at 200 \times g for 1 min and discard the flow-through.
 - 1.5 Perform step 1.4 two additional times.
 - 1.6 Insert the bottom cap.
 - 1.7 Immediately add the antibody solution (250 μ l) to the column.
 - 1.8 Seal the column with the lid.
 - 1.9 Fully resuspend the media, mix by inversion and make sure there is a flow in the column.
 - 1.10 Incubate the column with end-over-end mixing at room temperature for 2 h.
 - 1.11 Remove the bottom cap and place the column in a new microcentrifuge tube. Loosen the lid.
 - 1.12 Centrifuge at 1000 \times g for 1 min to collect the processed material.
 - 1.13 Insert the bottom cap. Add 100 μ l 1 \times TBS and seal the column with the lid.
 - 1.14 Invert the column a couple of times.
 - 1.15 Remove the bottom cap and place the column in a new microcentrifuge tube. Loosen the lid.
 - 1.16 Centrifuge at 1000 \times g for 1 min to collect the processed material.
 - 1.17 Repeat steps 1.13 to 1.16.
 - 1.18 Pool the collected fractions, including the sample from step 1.12 and adjust the sample volume to 550 μ l with 1 \times TBS.

2. Azide Activation

Time required: 5 min hands-on, followed by overnight incubation.

Materials from kit:

- 1× TBS (prepared from 20× TBS)
- UDP-GalNAz
- GalT enzyme
- Buffer additive

- 2.1 Add 7 µl Buffer additive to the pooled fractions from step 1.18.
- 2.2 Transfer the solution from step 2.1 to the GalT vial.
- 2.3 Reconstitute the UDP-GalNAz in 40 µl of 1× TBS and transfer the solution to the GalT vial.
- 2.4 Mix the solution by carefully pipetting up and down. Seal the vial with the lid and wrap the lid with Parafilm® or similar.
- 2.5 Incubate overnight protected from light at 30°C.

3. Removal of Excess UDP-GalNAz

Time required: 1 h.

Materials from kit:

- 1× TBS (prepared from 20× TBS)
 - Desalting Spin column (2 ml, 40K)
- 3.1 Let the Desalting Spin column (2 ml, 40K) equilibrate to room temperature before use. Twist off the bottom cap of the Desalting Spin column and place the column in a 15 ml centrifuge tube. Loosen the lid.
 - 3.2 Centrifuge at 700 × g for 2 min to remove the storage solution. Discard the flow-through.
 - 3.3 Place the column in the centrifuge tube.
 - 3.4 Add 1 ml 1× TBS on top of the resin. Centrifuge at 700 × g for 2 min and discard the flow-through.
 - 3.5 Perform step 3.4 two additional times. The last time, centrifuge for 3 min.
 - 3.6 Place the column in a new 15 ml centrifuge tube.
 - 3.7 Apply the azide-activated antibody sample from step 2.5 on top of the resin.
 - 3.8 Centrifuge at 700 × g for 3 min and collect the flow-through that contains the azide-activated antibody.
 - 3.9 At this stage, the azide-activated antibody can be stored at +4-8°C protected from light for conjugation of a label at a later time.

4. Conjugation with Biotin

Time required: 5 min hands-on, followed by overnight incubation.

Materials from kit:

- DIBO-modified label: Biotin

- 4.1 Reconstitute the DIBO-Biotin in 26 μ l DMSO per vial.
- 4.2 Transfer the azide-activated antibody in 1 \times TBS (from step 3.9) to a 1.5 ml microcentrifuge tube and add all of the DIBO-modified label from step 4.1. Mix the sample solution by carefully pipetting up and down.
- 4.3 Seal the tube with the lid and wrap the lid with Parafilm[®] or similar.
- 4.4 Incubate overnight protected from light at 25°C.
- 4.5 After the incubation, the antibody conjugate can be stored at +4-8°C, protected from light, until needed. **DO NOT FREEZE!** If preferred, sodium azide or thimerosal can be added to a final concentration of 0.02% (w/v) for long time storage.

5. Removal of Excess Biotin¹

Time required: 1 h.

Materials from kit:

- 1 \times TBS (prepared from 20 \times TBS) or other buffer of choice, for example PBS
 - Desalting Spin column (2 ml, 40K)
- 5.1 Let the Desalting Spin column (2 ml, 40K) equilibrate to room temperature before use. Twist off the bottom cap of the Desalting Spin column and place the column in a 15 ml centrifuge tube. Loosen the lid.
 - 5.2 Centrifuge at 700 \times g for 2 min to remove the storage solution. Discard the flow-through.
 - 5.3 Place the column in the centrifuge tube.
 - 5.4 Add 1 ml buffer on top of the resin. Centrifuge at 700 \times g for 2 min and discard the flow-through.
 - 5.5 Perform step 5.4 two additional times. The last time, centrifuge for 3 min.
 - 5.6 Place the column in a new 15 ml centrifuge tube.
 - 5.7 Apply the antibody conjugate sample (from step 4.5) on top of the resin.
 - 5.8 Centrifuge at 700 \times g for 3 min and collect the flow-through that contains the antibody conjugate.
 - 5.9 The antibody conjugate can now be stored protected from light at +4-8°C. **DO NOT FREEZE!** If preferred, sodium azide or thimerosal can be added to a final concentration of 0.02% (w/v) for long time storage.

1. This step is optional and dependent on your application.

CONTENT AND STORAGE

GlyCLICK Biotin 2 mg contains several components. The product is shipped cold, and the components should be stored at different temperatures upon arrival (see Table 1).

GlyCLICK Biotin is for R&D use only.

Table 1. Content and Storage Temperatures of GlyCLICK Components

Name	Amount	Store at
Desalting Spin column, 0.5 ml, 40K	1 piece	+4-8°C
Antibody concentrator 0.5 ml, 50K	1 piece	+4-25°C
Collection tube for antibody concentrator	2 pieces	+4-25°C
Desalting Spin column, 2 ml, 40K	2 pieces	+4-8°C
GlycINATOR Immobilized Microspin column	1 piece	+4-8°C
UDP-GalNAz	1 vial solid	+4-8°C Protect from light
20× TBS pH 7.4 (0.5 M)	2 × 2 ml	+4-8°C
Buffer additive	1 × 50 µl	+4-8°C Protect from light
β-1,4-galactosyltransferase GalT (Y289L)	1 × 40 µl	+4-8°C Protect from light
DIBO-modified label: Biotin	2 vials solid	(-25)-(-5)°C Protect from light

USA & Canada

Genovis Inc.

10919 Technology Place Suite C, San Diego, CA 92127, USA

Phone: 1-855-782-0084 (toll free)

Fax: 1-858-524-3006

EMEA & Asia

Genovis AB

Box 4, SE-24421 Kävlinge, Sweden

Phone: +46 46 10 12 30

Fax: +46 46 12 80 20

support@genovis.com

www.genovis.com



All rights reserved. Genovis products may be covered by one or more patents, trademarks and copyrights owned or controlled by Genovis AB. For more information about commercial rights, please contact the Genovis team at licensing@genovis.com.

Genovis products are intended for research use only. They are not intended to be used for therapeutic or diagnostic purposes in humans or animals.

All goods and services are sold subject to Genovis' General Terms and Conditions of Sale.

SiteClick™ is provided under an intellectual property license from Life Technologies Corporation. The transfer of this product is conditioned on the buyer using the purchased product solely in research conducted by the buyer, excluding contract research or any fee for service research, and the buyer must not (1) use this product or its components for (a) diagnostic, therapeutic or prophylactic purposes; (b) testing, analysis or screening services, or information in return for compensation on a per-test basis; or (c) manufacturing or quality assurance or quality control, and/or (2) sell or transfer this product or its components for resale, whether or not resold for use in research. For information on purchasing a license to this product for purposes other than as described above, contact Life Technologies Corporation, 5791 Van Allen Way, Carlsbad, CA 92008 USA or outlicensing@lifetech.com.

The trademark SiteClick™ is the property of Life Technologies Corporation.

© Genovis AB